

NEW

## Fluorescence lifetime spectrometer C16361 series



**HAMAMATSU**  
PHOTON IS OUR BUSINESS



Quantaurus-Tau® is a compact system for measuring fluorescence lifetimes in the sub-nanosecond to millisecond range. Operation is simple, just set the sample into the sample chamber, and enter a few conditions on the measurement software to measure the fluorescence lifetime and PL spectrum in a short time with high precision.

In a typical measurement, analysis results are obtained in a mere 60 seconds.

## ● Easy and quick measurements

Emission lifetime can be gotten easily and quickly only by putting the sample into sample box and setting the 4 measurement conditions.

## ● 7 excitation wavelengths


280 nm, 340 nm, 365 nm, 405 nm, 470 nm, 590 nm, and 630 nm.

## ● Analyzing different sample forms

Thin-film, solid, solutions and powder.

## ● 2 selections of detector

### Detector spectral sensitivity

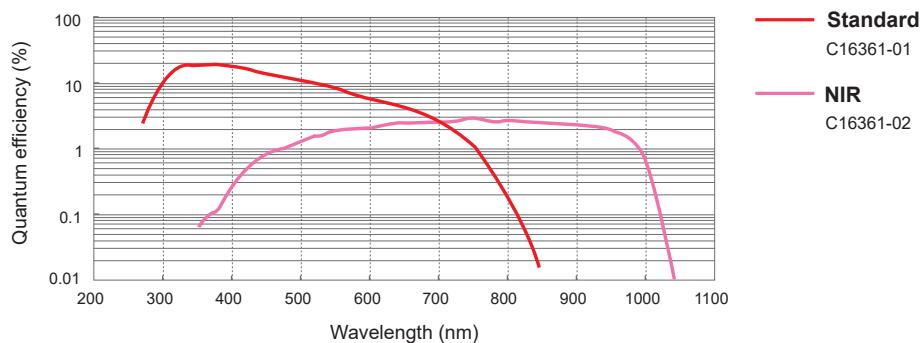


# Capable of measuring various fluorescence lifetimes

The fluorescence spectrum obtained from an organic material or fluorescent probe is a vital parameter for controlling and evaluating the material functions and characteristics such as the peak wavelength and fluorescence intensity. However, a fluorescence spectrum usually shows time-integrated information, and so when the material contains multiple substances and reactive elements, their fluorescence spectrum can only be acquired as integrated information. An effective approach in such cases is to observe the light emission dynamics by making use of the time axis parameter. This is generally called fluorescence lifetime measurement, in which the time required for the substance excited by the pulsed light to return to its ground state is measured in the sub-nanosecond to millisecond region. This measurement allows obtaining more information such as multiple different fluorescence lifetimes even at the same wavelength and the percentage in which they are present within the material, etc.

## Basic functions of fluorescence lifetime measurement


- **High sensitivity measurement by photon counting method (TCSPC\*)**
  - \* Time correlated single photon counting
- **Time resolution better than 100 ps (by deconvolution)**
- **Cooling function for solution sample (-196 °C) (option)**
- **Phosphorescence measurement (option)**
- **Fluorescence spectrum measurement**

## Application to fluorescence lifetime

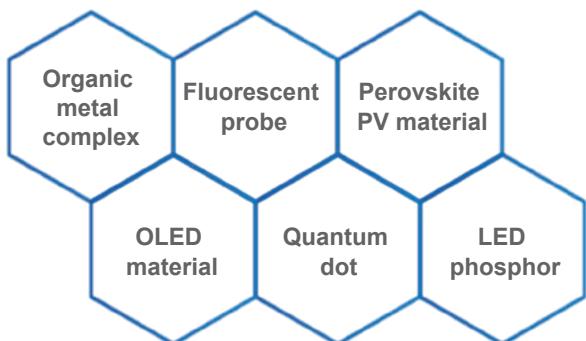


Fluorescence lifetime measurement is applicable to varied applications. Typical applications include electron movement and energy transfer reactions within or between organic metallic complex molecules, as well as fluorescence and phosphorescence lifetime measurement of materials essential for developing organic EL devices, FRET (fluorescence resonance energy transfer) in fluorescent proteins, and pass/fail testing of compound semiconductors for solar cells and LED, etc.

# The software takes account of the measurement procedure ensuring quick and easy measurements.

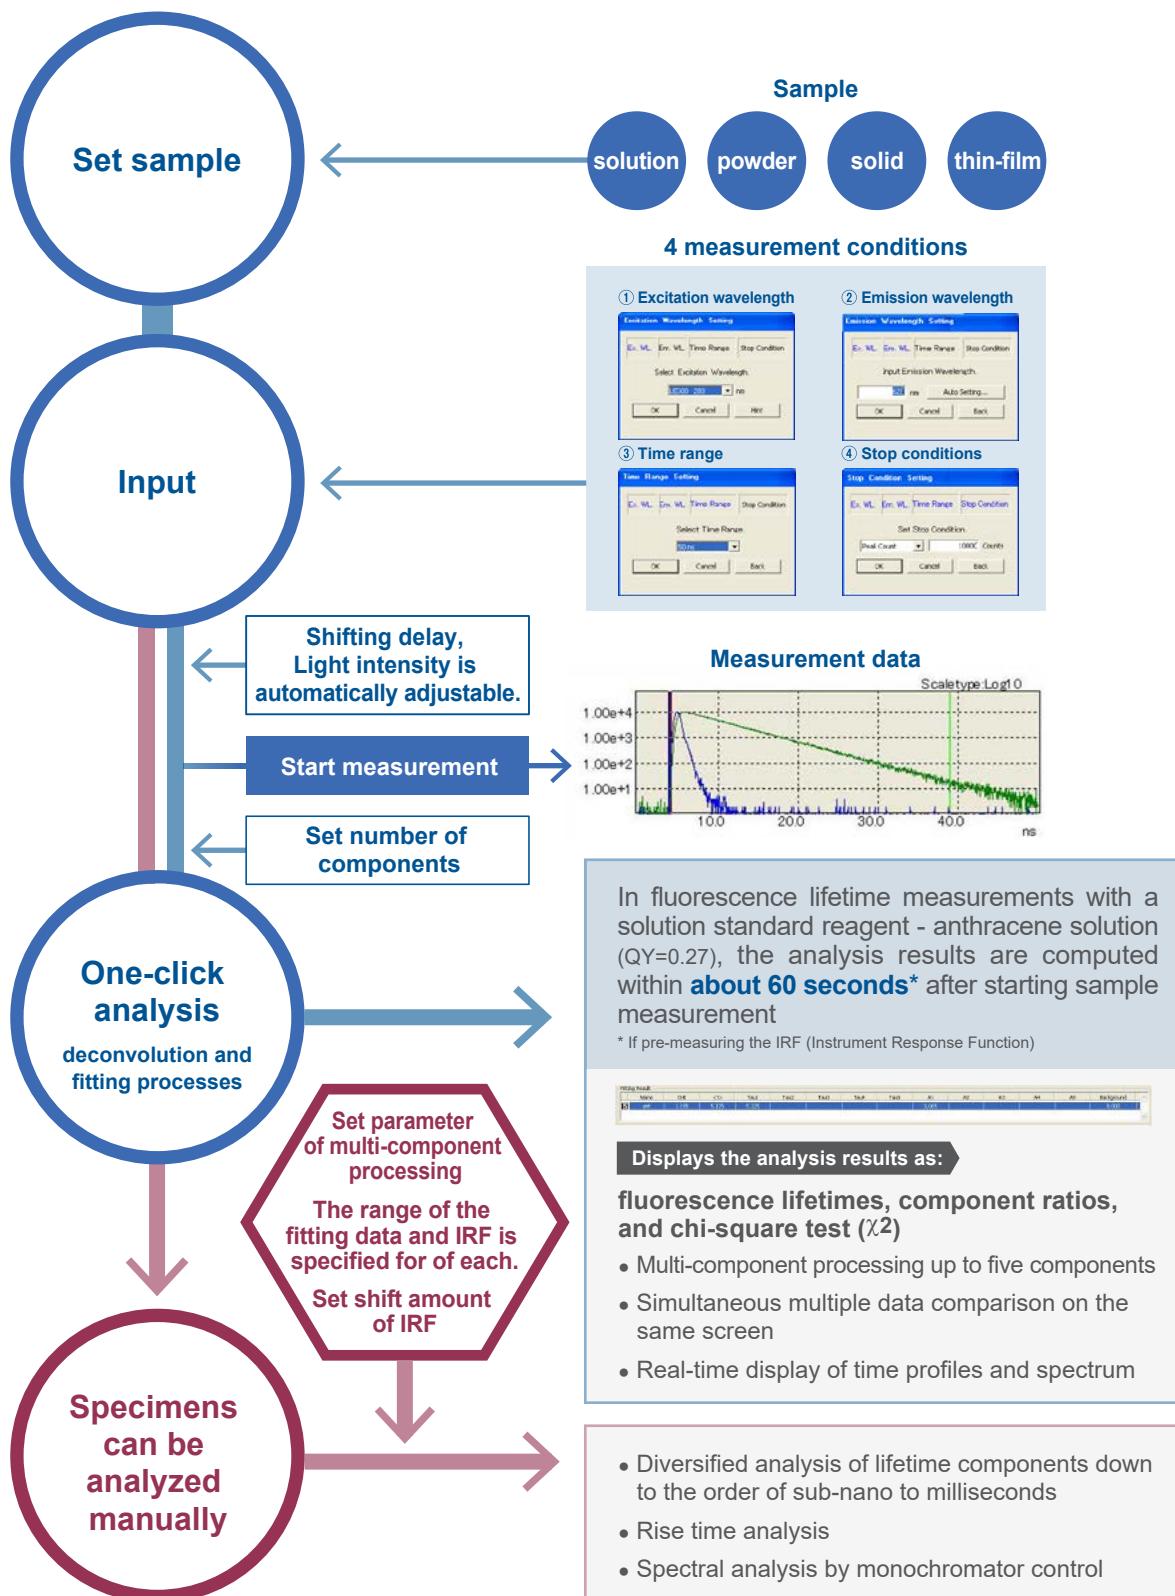

**Quantaurus-Tau® includes a variety of measurement and analysis functions such as simultaneous multi-component fluorescence lifetime measurement and multi-sample data comparison.**

### ● Multi-component fluorescence lifetime analysis and comparison

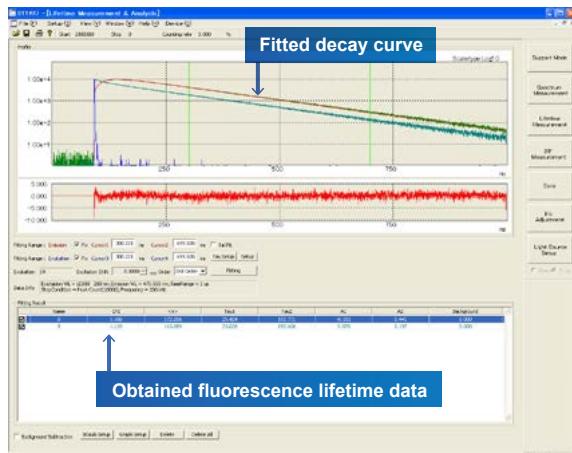

- **Multi-component analysis of up to five components**

In fluorescence lifetime measurement, a phenomenon often occurs where the data is observed as the sum of the attenuation curves of multi-component fluorescence lifetimes. Quantaurus-Tau® easily calculates the fluorescence lifetime data and component ratio of each element by using the dedicated software.


- **Highly accurate analysis by deconvolution**

Deconvolution processing enables fluorescence lifetime analysis with high accuracy. When analyzing longer lifetime components such as phosphorescence, the "Tail Fit" function can be used instead of deconvolution processing.

- **Real-time display of time profiles and spectrum**

Time profiles or spectrum are displayed on the monitor screen in real-time. This is a useful function for selecting the time scale during measurement or determining the analysis data range.

### ● Multi-sample fluorescence lifetime analysis and comparison

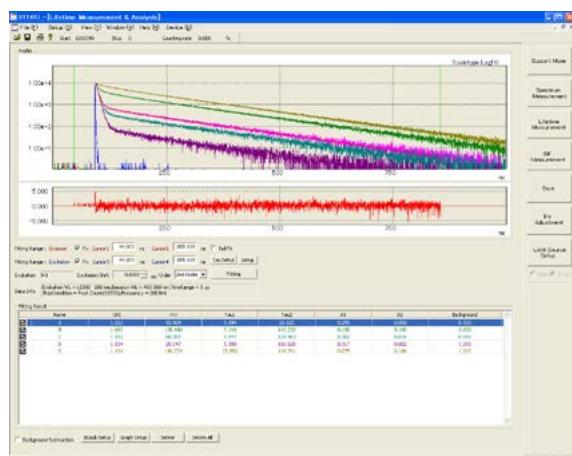

- **Multiple data analysis on the same screen**

Calculated fluorescence lifetime values are also displayed on the same screen for easy comparison analysis.

- **Comparisons under the same fitting conditions**

To make comparison analysis under the same conditions, Quantaurus-Tau® subjects the multiple samples to specific fitting ranges, IRF (Instrument Response Function), and parameter settings.


- **Graph editing with a graph setup feature**

This allows you to change the range of each axis as needed on the comparison analysis screen so that the data can be edited to match your purpose. This feature also allows powerful normalizing whenever needed.

- **Acquired data can be easily stored as text data**

The acquired data can be stored into the graph analysis software as text data by simple copy-and-paste operations.

### ● Multi-sample PL spectrum analysis and comparison

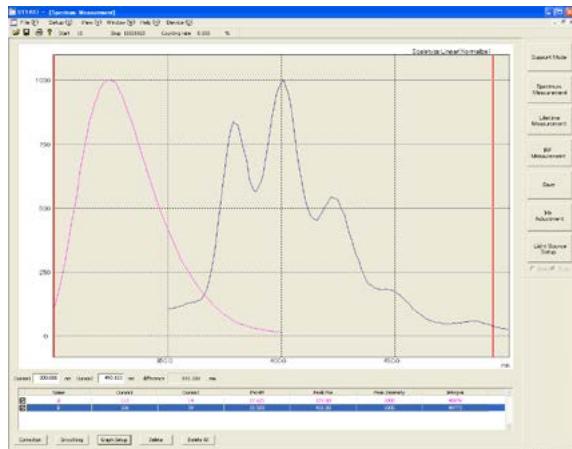

- **Time-resolved spectrum display**

Allows time-resolved spectrum display the greatest feature offered by streak camera systems.

- **Spectrum and fluorescence decay curve display**


Displays the full width at half maximum (FWHM), peak position and peak intensity for each profile.

- **Multiple data loading and comparison on the same screen**


Normalized processing makes multiple data comparison easy.

# Our long and proven record in fluorescence lifetime measurements is the reason our products are favored by many users in a wide range of fields.


## TADF of the blue OLED material

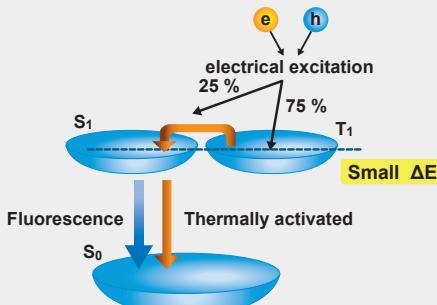

TADF (Thermally activated delayed fluorescence) is known well as the 3rd generation OLED material which is high efficiency and cost saving, furthermore can be replaced with phosphorescence material. The data shows the example of fluorescence lifetime measurement of blue TADF material. In order to achieve the high efficiency, the molecule design is the important factor to minimize the energy gap of excited singlet state ( $S_1$ ) and excited triplet state ( $T_1$ ).

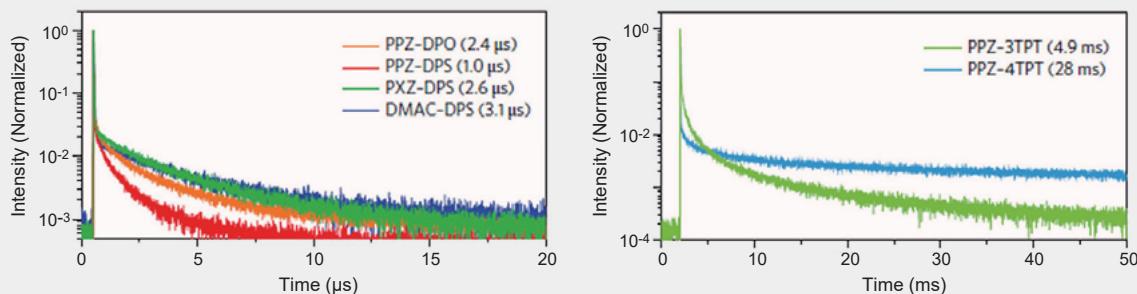

Delayed fluorescence of TADF material results in that small gap of  $\Delta E_{st}$ , which is defined as the energy gap of  $S_1$  state and  $T_1$  state, is in the microsecond range. On the other hand, wide gap of  $\Delta E_{st}$  is in millisecond range.

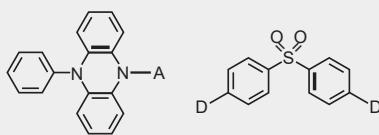


A= PPZ-DPO,  
PPZ-3TPT, PPT-4TPT  
D=PPZ-DPS, PXZ-DPS,  
DMAC-DPS

PPZ: 5-phenyl-5,10-dihydrophenazine  
DPO: 2,5-diphenyl-1,3,4-oxadiazole  
TPT: 3,4,5-triphenyl-1,2,4-triazole  
DPS: diphenylsulphone  
PXZ: phenoxazine  
DMAC: 9,9-dimethyl-9,10-dihydroacridine


Data courtesy of Prof. Chihaya Adachi, Hajime Nakanotani  
Center for Organic Photonics and Electronics Research, Kyushu Univ.

Q. Zhang, B. Li, S. Huang, H. Nomura, H. Tanaka and C. Adachi, *nature photonics*, **8**, 326 (2014)

## Temperature dependency of fluorescence lifetime with TADF material

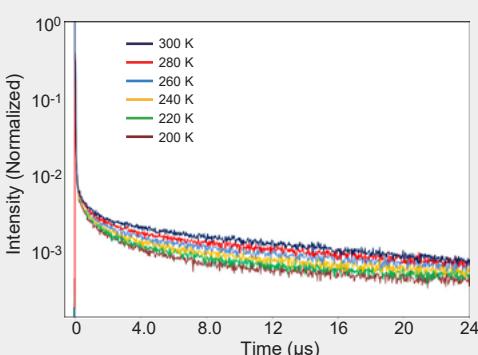

Temperature dependence of transient PL decays of triarylboron-based OLED emitter doped in CBP (16 wt%).



The fluorescence lifetime measurement example to observe the temperature dependency of triarylboron-based compound which is the TADF material. Phosphorescence material as the typical OLED material has chemical behavior to decrease the ratio of the light components by the temperature increasing. As the temperature rose, TADF material, however, increased the delayed fluorescence components and resulted the delay components were activated by the heat. The temperature dependency measurement was done with the setup of Cryostat.

Data courtesy of Prof. Hironori Kaji, Atsushi Wakamiya, Katsuaki Suzuki, Institute for Chemical Research, Kyoto Univ.  
Data courtesy of Prof. Chihaya Adachi, Center for Organic Photonics and Electronics Research, Kyushu Univ.

K. Suzuki, S. Kubo, K. Shizu, T. Fukushima, A. Wakamiya, Y. Murata, C. Adachi, H. Kaji, *Angew chem. Int. Ed.* **54**, 15231 (2015).

# We also offer a lineup of quantum yield measurement systems allowing diversified material evaluations on the same sample.

## Fluorescence Lifetime and Absolute PL Quantum Yield

There are two processes when substances are excited by light irradiation from the ground state to excited singlet state ( $S_1$ ), then deactivated to the ground state again. One is radiative process such as fluorescence and the other is a non-radiative process released as heat.

The fluorescence lifetime  $\tau$  (tau) is defined as

$$k_f + k_{nr} = 1 / \tau$$

where  $k_f$  is the radiative rate constant and  $k_{nr}$  is the non-radiative constant.

On the other hand, the PL Quantum Yield ( $\Phi$ ) is expressed as the ratio of the number of photons emitted from molecules ( $PN_{em}$ ) to that absorbed by molecules ( $PN_{abs}$ ).

$$\Phi = PN_{em} / PN_{abs}$$

The PL Quantum Yield  $\Phi$  is also written as

$$\Phi = k_f / (k_f + k_{nr})$$

Thus, there is a correlation between  $\tau$  (tau) and  $\Phi$  as shown in the following equation, and they are very important parameters for controlling the emission mechanisms of the materials.

$$k_f = \Phi / \tau$$




## A diversified evaluation of the luminescence materials is available!

Quantaurus-Tau® for measuring fluorescence lifetime and Quantaurus-QY® for absolute PL quantum yield with simplified and minimized operating procedure are available.

Combination of Quantaurus-Tau® and Quantaurus-QY® allow users to obtain complementary analysis results.

### ff luminescent characteristic of Lanthanide complex

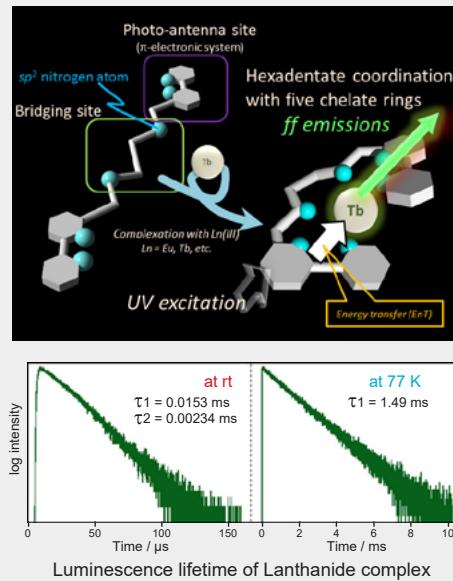

Lanthanide compound has a characteristic of high luminescent performance and is expected to apply for the variety of functional materials such as OLED, photovoltaic or a sensor.

The fluorescence lifetime of a series of Lanthanide complex was measured in the acetonitrile solution (at room temperature) and the solid state (at room temperature, at 77K). A series of Lanthanide complex has Bipyridine skeleton.

The remarkable difference was observed to fluorescence lifetime depending on the temperature ( $\tau$ ) and Quantum yield (QY) of  $Tb^{III}$  complex which has the characteristic of thermal equilibrium caused by the energy transfer between excited triplet state of ligand and the energy level of center metal.

	Temp.	$\tau$ [ms](amp.)	QY <sup>a</sup> [%]
EuL	In the solid state	rt 77 K	1.27 (1.0) 1.35 (1.0)
	In acetonitrile	rt 77 K	1.55 (1.0) 0.0153 (0.96)
TbL	In the solid state	rt 77 K	0.00234 (0.04) 1.49 (1.0)
	In acetonitrile	rt n.d.	1.0 (±0.2) 91.5 (±1.4) ≈ 0

<sup>a</sup> The values of  $Ln$  emission were based on the ligand excitation, and observed with Absolute PL quantum yield spectrometer C9920-02.

Data courtesy of Prof. Miki Hasegawa, Aoyama Gakuin Univ.

M. Hasegawa, H. Ohtsu, D. Kodama, T. Kasai, S. Sakurai, A. Ishii, and K. Suzuki, *New J. Chem.*, **38**, 1225 (2014)

L: Ligand

amp.: amplitude

rt: room temperature

## Specifications

Type number	C16361-01	C16361-02
Detector type	Standard	NIR
Wavelength range	300 nm to 800 nm	380 nm to 1030 nm
Excitation light source	Seven types of LED light source (280 nm, 340 nm, 365 nm, 405 nm, 470 nm, 590 nm, 630 nm)	
Excitation light source switching		Software control
Monochromator		Czerny-Turner monochromator
Measurement time range		4 ns to 10 s / full scale
Time range for phosphorescence measurement		200 μs to 10 s / full scale (option)
Phosphorescence measurement	Phosphorescence excitation wavelength (280 nm, 340 nm, 365 nm, 405 nm, 442 nm, 470 nm, 589 nm, 632 nm)	
Time axis channel	512 ch, 1024 ch, 2048 ch, 4096 ch	
Total time resolution	< 1.0 ns FWHM (IRF with 590 nm LED)	
Analysis function	Fluorescence lifetime analysis (up to five components by exponential function fitting) and spectrum analysis	
Supported OS		Windows® 10 (64 bit)

## Options

### Sample box

#### Sample box for solution sample A16362-01

A16362-01 is a sample box for measuring the solution samples (compatible with 10 mm square cells) or thin film samples.

#### Sample box for solid sample A16362-02

A16362-02 is a sample box for measuring the powder samples or thin solid film samples.

#### Sample box for Low-temperature A11797-02

A11797-02 is a sample box for setting A11238-04 when measuring the lifetime of a solution samples at liquid nitrogen temperature.

#### Sample box for cryostat Optistat DN A12268-01

Sample box for Optistat DN2 (Oxford Instruments).

### Sample holder

#### Sample holder for low temperature A11238-04

This is used to cool the solution sample with liquid nitrogen.

### Sample case

#### For solution Side-arm cell (3 pieces) A10095-02

##### Sample tube for low temperature measurement (5 pieces) A10095-04

This is used to measure a sample solution at liquid nitrogen temperature.

#### For powder Laboratory dish without caps (5 pieces) A10095-01

##### Laboratory dish with caps (5 pieces) A10095-03

This is used for making measurements on powder samples. This contains 5 dishes made of synthetic quartz, which suppresses fluorescence and luminescence.



##### Tweezers for A10095-03 A13712

Tweezers for grasping petri dishes.

### Light source option

#### Xenon flash lamp unit For Phosphorescence measurement C11567-02

C11567-02 is the excitation light source using Xenon flash lamp for phosphorescence measurement from a few tens of microseconds to milliseconds.

#### Band pass filter A12991- 280

Band pass filter for the wavelength 280 nm.

#### Band pass filter A13905- XXX

Selectable from among the following wavelengths: 340 nm, 365 nm, 405 nm, 442 nm, 470 nm, 589 nm, 632 nm.

#### PLP-10-XXXTAU Laser diode head M12488 series


M12488 series are the dedicated laser diode heads for Quantaurus-Tau®, which can be used in combination with the controller and adapter.

Selectable from the following wavelength of 375 nm, 405 nm, 445 nm, 465 nm, 483 nm, 510 nm, 655 nm, 785 nm, 850 nm.

#### Adapter A12487-01

A12487-01 is an adapter for attaching M12488 to Quantaurus-Tau®. A12487-01 is used when excitation light source is the PLP-10.

### Dimensional outlines (unit: mm) Weight: 31 kg

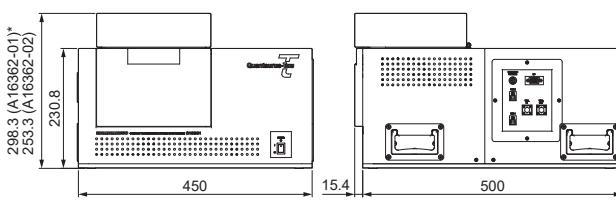

\* The height is changed by sample box type.

★ Quantaurus-QY is registered trademark of Hamamatsu Photonics K.K. (China, EU, Japan, Korea, U.K., U.S.A.)

Quantaurus-Tau is registered trademark of Hamamatsu Photonics K.K. (China, EU, Japan, Korea, U.K.)

Windows is registered trademark of Microsoft Corporation in the U.S.A.

Product and software package names noted in this documentation are trademarks or registered trademarks of their respective manufacturers.

- Subject to local technical requirements and regulations, availability of products included in this promotional material may vary. Please consult your local sales representative.
- Information furnished by HAMAMATSU is believed to be reliable. However, no responsibility is assumed for possible inaccuracies or omissions.

Specifications and external appearance are subject to change without notice.

© 2022 HAMAMATSU PHOTONICS K.K.

**HAMAMATSU PHOTONICS K.K.** [www.hamamatsu.com](http://www.hamamatsu.com)

Systems Division

812 Joko-cho, Higashi-ku, Hamamatsu City, 431-3196, Japan, Telephone: (81)53-431-0124, Fax: (81)53-433-8031, E-mail: export@sys.hpk.co.jp

U.S.A.: HAMAMATSU CORPORATION: 360 Foothill Road, Bridgewater, NJ 08807, U.S.A., Telephone: (1)908-231-0960, Fax: (1)908-231-1218 E-mail: usa@hamamatsu.com

Germany: HAMAMATSU PHOTONICS DEUTSCHLAND GMBH.: Arzbergerstr. 10, 82211 Herrsching am Ammersee, Germany, Telephone: (49)8152-375-0, Fax: (49)8152-265-8 E-mail: info@hamamatsu.de

France: HAMAMATSU PHOTONICS FRANCE S.A.R.L.: 19, Rue du Saule Trapu, Parc du Moulin de Massy, 91882 Massy Cedex, France, Telephone: (33)1 69 53 71 10 E-mail: infos@hamamatsu.fr

United Kingdom: HAMAMATSU PHOTONICS UK LIMITED: 2 Howard Court, 10 Twin Road, Welwyn Garden City, Hertfordshire AL7 1BW, UK, Telephone: (44)1707-294888, Fax: (44)1707-325777 E-mail: info@hamamatsu.co.uk

North Europe: HAMAMATSU PHOTONICS NORDEN AB: Torshamngatan 35 16440 Kista, Sweden, Telephone: (46)8-509 031 00, Fax: (46)8-509 031 01 E-mail: info@hamamatsu.se

Italy: HAMAMATSU PHOTONICS ITALIA S.R.L.: Strada della Moia, 1 Int. 6, 20044 Arese (Milano), Italy, Telephone: (39)02-93 58 17 33, Fax: (39)02-93 58 17 41 E-mail: info@hamamatsu.it

China: HAMAMATSU PHOTONICS (CHINA) CO., LTD.: 1201 Tower B, Jiaming Center, 27 Dongsanhuai Beilu, Chaoyang District, 100020 Beijing, P.R. China, Telephone: (86)10-6586-6006, Fax: (86)10-6586-2866 E-mail: hpc@hamamatsu.com.cn

Taiwan: HAMAMATSU PHOTONICS TAIWAN CO., LTD.: 8F-3, No.158, Section 2, Gongdao 5th Road, East District, Hsinchu, 300, Taiwan R.O.C., Telephone: (886)3-659-0080, Fax: (886)3-659-0081 E-mail: info@hamamatsu.com.tw

Cat. No. SHSS0025E02  
MAR/2022 HPK  
Created in Japan